

FUGRO TECHNICAL SERVICES LIMITED

Fugro Development Centre,
5 Lok Yi Street, Tai Lam,
Tuen Mun, N.T.,
Hong Kong.

Tel : +852 2450 8233
Fax : +852 2450 6138
E-mail : matlab@fugro.com.hk
Website : www.materialab.com.hk

Materialab

Report no.: 940891CA160442(1)

Page 1 of 1

CALIBRATION CERTIFICATE OF SOUND CALIBRATOR

Client : Fugro Technical Services Ltd.

Project : Calibration Services

Client Supplied Information

Details of Unit Under Test, UUT

Description : Sound Calibrator
Manufacturer : Casella (Model no. CEL-120/1)
Serial No. : 5230742
Next Calibration Date : 02-Mar-2017
Specification Limit : ± 0.5 dB

Laboratory Information


Description : Reference Sound Level Meter
Equipment ID. : R-119-1
Date of Calibration : 03-Mar-2016 Ambient Temperature : 21 °C
Calibration Location : Calibration Laboratory of Materialab
Method Used : By direct comparison

Calibration Results :

Parameters (Setting of UUT)	Mean Value (error of measurement)	Specification Limit(dB)
94dB	-0.1 dB	± 0.5 dB
114dB	-0.3 dB	

Remarks :

1. The equipment used in this calibration is traceable to recognized National Standards.
2. The mean value is the average of four measurements.
3. The equipment does comply with specification limit.

Checked by : 
CA-R-297 (22/07/2009)

Date : 4.3.2016

Certified by :



Date : 07 MAR 2016

Kwok Chi Wa (Assistant Manager)

** End of Report **

FUGRO TECHNICAL SERVICES LIMITED

Fugro Development Centre,
5 Lok Yi Street, Tai Lam,
Tuen Mun, N.T.,
Hong Kong.

Tel : +852 2450 8233
Fax : +852 2450 6138
E-mail : matlab@fugro.com
Website : www.materialab.com

MaterialLab

Report no.: 161966CA160797

Page 1 of 1

CALIBRATION CERTIFICATE OF SOUND CALIBRATOR

Client : MaterialLab Consultants Ltd.

Address : Room 723 & 725, 7F., Block B Profit Industrial Building, 1-15 Kwai Fung Crescent, Kwai Chung, N.T.

Project : Calibration Services

Client Supplied Information

Details of Unit Under Test, UUT

Description : Sound Calibrator
Manufacturer : Casella (Model no. CEL-120/1)
Serial No. : 5230736
Next Calibration Date : 20-Apr-2017
Specification Limit : $\pm 0.5\text{dB}$

Laboratory Information



Description : Reference Sound Level Meter
Equipment ID. : R-119-1
Date of Calibration : 21-Apr-2016 Ambient Temperature : 21 °C
Calibration Location : Calibration Laboratory of MaterialLab
Method Used : By direct comparison

Calibration Results :

Parameters (Setting of UUT)	Mean of Measured value	Specification Limit(dB)
94dB	93.9 dB	$\pm 0.5\text{dB}$
114dB	114.1 dB	

Remarks :

1. The equipment used in this calibration is traceable to recognized National Standards.
2. The mean value is the average of four measurements.
3. The equipment does comply with specification limit.

Checked by :  Date : 22/4/2016 Certified by :  Date : 22 APR 2016

CA-R-297 (22/07/2009)

Kwok Chi Wa (Assistant Manager)

** End of Report **

Certificate of
Conformance and Calibration for**CEL-120 Acoustic Calibrator**

Applicable Standards :- IEC 60942: 2003 & ANSI S1.40: 2006

CEL-120/1 Class 1 CEL-120/2 Class 2 Serial No: 4358251Firmware: 03Temperature: 22.0 °C Pressure: 999.5 mb %RH 55.0

Frequency = 1.00kHz ± 2Hz T.H.D. = < 1%	Calibration Level
SPL @ 114.0dB Setting	<u>113.99</u> dB
SPL @ 94.0dB Setting (CEL-120/1 only)	<u>93.93</u> dB/N.A

Engineer :- M. Duncanson Date :- 12 MAY 2016

Company test equipment and acoustic working standards, used for conformance testing, are subject to periodic calibration, traceable to UK national standards, in accordance with the company's ISO9001 Quality System.

DECLARATION OF CONFORMITY

This certificate confirms that the instrument specified above has been produced and tested to comply with the manufacturer's published specifications and the relevant European Community CE directives.

Casella CEL (U.K.),
Regent House, Wolsley Road, Kempston, Bedford, MK42 7JY
Phone: +44 (0) 1234 844100 Fax: +44 (0) 1234 841490
E-mail: info@casellacel.com
Web: www.casellameasurement.com

198032A-01

Certificate of Conformity and Calibration

Instrument Model:- CEL-633A
 Serial Number 3756127
 Firmware revision V129-09

Microphone Type:- CEL-251
 Serial Number 1231

Preamplifier Type:- CEL-495
 Serial Number 003036

Instrument Class/Type:- 1



Applicable standards:-

IEC 61672: 2002 / EN 60651 (Electroacoustics - Sound Level Meters)
 IEC 60651 1979 (Sound Level Meters), ANSI S1.4: 1983 (Specifications For Sound Level Meters)

Note:- The test sequences performed in this report are in accordance with the current Sound level meter Standard - IEC61672. The combination of tests performed are considered to confirm the products electro-acoustic performance to all applicable standards including superceeded Sound Level Meter Standards - IEC60651 and IEC60804.

Test Conditions:- 25 °C
 52 %RH
 1010 mBar

Test Engineer:- Millie Duncan
Date of Issue:- February 2, 2016

Declaration of conformity:-

This test certificate confirms that the instrument specified above has been successfully tested to comply with the manufacturer's published specifications. Tests are performed using equipment traceable to national standards in accordance with Casella's ISO 9001:2008 quality procedures. This product is certified as being compliant to the requirements of the CE Directive.

Test Summary:-

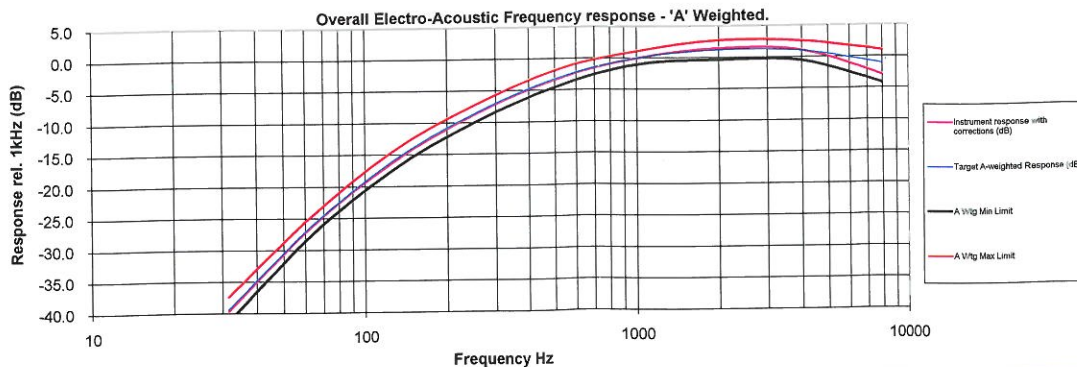
- Self Generated Noise Test
- Electrical Signal Test Of Frequency Weightings
- Frequency & Time Weightings At 1 kHz
- Level Linearity On The Reference Level Range
- Toneburst Response Test
- C-peak Sound Levels
- Overload Indication
- Acoustic Tests

- All Tests Pass
- All Tests Pass
- All Tests Pass
- All Tests Pass
- All Tests Pass
- All Tests Pass
- All Tests Pass
- All Tests Pass

Combined Electro-Acoustic Frequency Response - A Weighted

Combined Electro-Acoustic Frequency Response - A Weighted (IEC 61672-3:2006)

The following A-Weighted frequency response graph shows this instruments overall frequency response based upon the application of multi-frequency pressure field calibrations. The microphones Pressure to Free field correction coefficients are applied to pressure response. Reference level taken at 1kHz.



Casella CEL
 Regen House, Wolsley Road,
 Kempston, Bedford
 MK42 7JY
 Phone: +44(0) 1234 844100
 Fax: +44(0) 1234 841490
 E-mail: info@casellameasurement.com
 Web: www.casellameasurement.com

Casella CEL, Inc. a subsidiary of IDEAL Industries, Inc.
 415 Lawrence Bell Drive
 Unit 4
 Buffalo, NY 14221
 Toll Free: (800) 366-2966
 Tel: (603) 672-0031 Fax: (603) 672-8053
 E-mail: info@casellausa.com
 Web: www.casellausa.com

Certificate of Conformity and Calibration

Instrument Model:- CEL-633A
Serial Number 3756084
Firmware revision V129-09

Microphone Type:- CEL-251
Serial Number 1257

Preamplifier Type:- CEL-495
Serial Number 003538

Instrument Class/Type:- 1



Applicable standards:-

IEC 61672: 2002 / EN 60651 (Electroacoustics - Sound Level Meters)
 IEC 60651 1979 (Sound Level Meters), ANSI S1.4: 1983 (Specifications For Sound Level Meters)

Note:- The test sequences performed in this report are in accordance with the current Sound level meter Standard - IEC61672. The combination of tests performed are considered to confirm the products electro-acoustic performance to all applicable standards including superceded Sound Level Meter Standards - IEC60651 and IEC60804.

Test Conditions:- 25 °C
 52 %RH
 1010 mBar

Test Engineer:- Millie Duncan
Date of Issue:- February 2, 2016

Declaration of conformity:-

This test certificate confirms that the instrument specified above has been successfully tested to comply with the manufacturer's published specifications. Tests are performed using equipment traceable to national standards in accordance with Casella's ISO 9001:2008 quality procedures. This product is certified as being compliant to the requirements of the CE Directive.

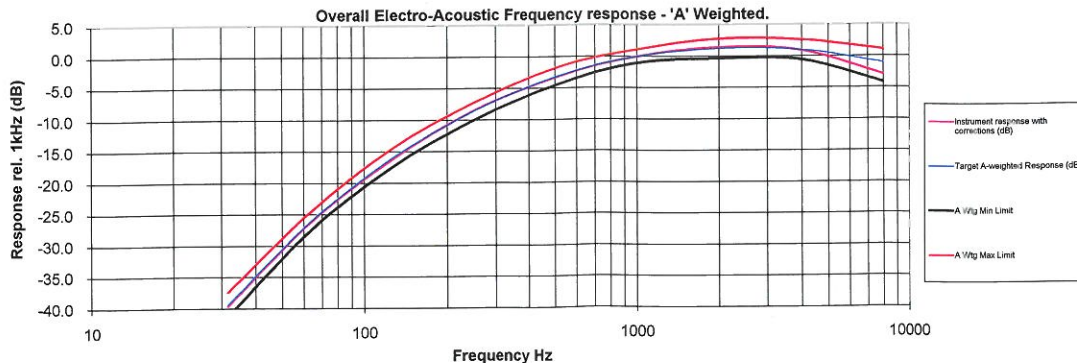
Test Summary:-

Self Generated Noise Test	All Tests Pass
Electrical Signal Test Of Frequency Weightings	All Tests Pass
Frequency & Time Weightings At 1 kHz	All Tests Pass
Level Linearity On The Reference Level Range	All Tests Pass
Toneburst Response Test	All Tests Pass
C-peak Sound Levels	All Tests Pass
Overload Indication	All Tests Pass
Acoustic Tests	All Tests Pass

Combined Electro-Acoustic Frequency Response - A Weighted

Combined Electro-Acoustic Frequency Response - A Weighted (IEC 61672-3:2006)

The following A-Weighted frequency response graph shows this instruments overall frequency response based upon the application of multi-frequency pressure field calibrations. The microphones Pressure to Free field correction coefficients are applied to pressure response. Reference level taken at 1kHz.



Casella CEL
 Regen House, Wolseley Road,
 Kempston, Bedford
 MK42 7JY
 Phone: +44(0) 1234 844100
 Fax: +44(0) 1234 841490
 E-mail: info@casellameasurement.com
 Web: www.casellameasurement.com

Casella CEL, Inc. a subsidiary of IDEAL Industries, Inc.
 415 Lawrence Bell Drive
 Unit 4
 Buffalo, NY 14221
 Toll Free: (800) 366-2966
 Tel: (603) 672-0031 Fax: (603) 672-8053
 E-mail: info@casellausa.com
 Web: www.casellausa.com

FUGRO TECHNICAL SERVICES LIMITED

Fugro Development Centre,
5 Lok Yi Street, Tai Lam,
Tuen Mun, N.T.,
Hong Kong.

Tel : +852 2450 8233
Fax : +852 2450 6138
E-mail : matlab@fugro.com.hk
Website : www.materialab.com.hk

Materialab

Report no.: 940891CA152019(1)

Page 1 of 1

CALIBRATION CERTIFICATE OF SOUND LEVEL METER

Client : Fugro Technical Services Ltd.

Project : Calibration Services

Client Supplied Information

Details of Unit Under Test, UUT

Description : Sound Level Meter
Manufacturer : Casella (Model no. CEL-63X(meter), CEL-251(microphone), CEL-495(Preamplifier))
Serial No. : 3321823 (meter), 2058 (microphone), 001598 (Preamplifier)
Next Calibration Date : 14-Oct-2016
Specification Limit : EN 60651: 1994 Type 1

Laboratory Information


Description : B & K Acoustic Multifunction Calibrator 4226 (Traditional free field setting)
Equipment ID. : R-108-1
Date of Calibration : 15-Oct-2015 Ambient Temperature : 20 °C
Calibration Location : Calibration Laboratory of Materialab
Method Used : By direct comparison

Calibration Results :

Parameters		Mean Value (dB)	Specification Limit(dB)
A-weighting frequency response	4000Hz	0.6	2.0 to 0.0
	2000Hz	1.1	2.2 to 0.2
	1000Hz	0.0	1.0 to -1.0
	500Hz	-3.2	-2.2 to -4.2
	250Hz	-8.6	-7.6 to -9.6
	125Hz	-16.0	-15.1 to -17.1
	63Hz	-26.0	-24.7 to -27.7
	31.5Hz	-38.9	-37.9 to -40.9
Differential level linearity	94dB-104dB	0.0	± 0.4
	104dB-114dB	0.1	± 0.4

Remarks :

1. The equipment used in this calibration is traceable to recognized National Standards.
2. The mean value is the average of four measurements.
3. For calibration: Reference SPL are 94, 104 & 114dB, range setting is 20-140dB & time weighing is fast
4. The equipment does comply with EN 60651: 1994 Type 1 sound level meter for the above measurement.

Checked by : 
CA-R-297 (22/07/2009)

Date : 15/10/2015

Certified by : 

So Chi Kuen (Engineer)

Date : 15 Oct, 2015

** End of Report **